

FIG. 1

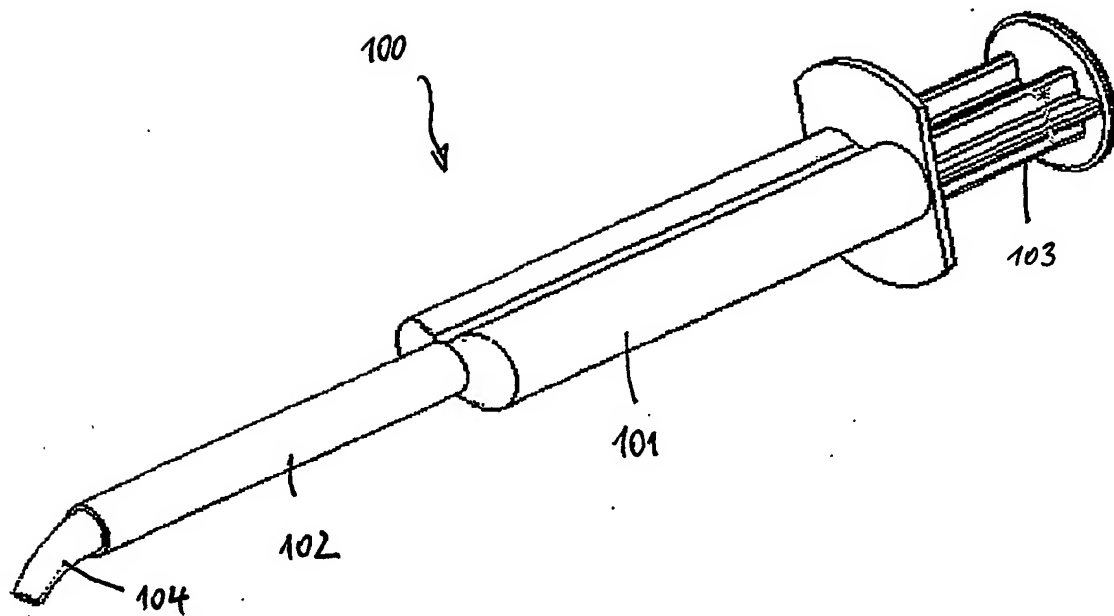


FIG. 2

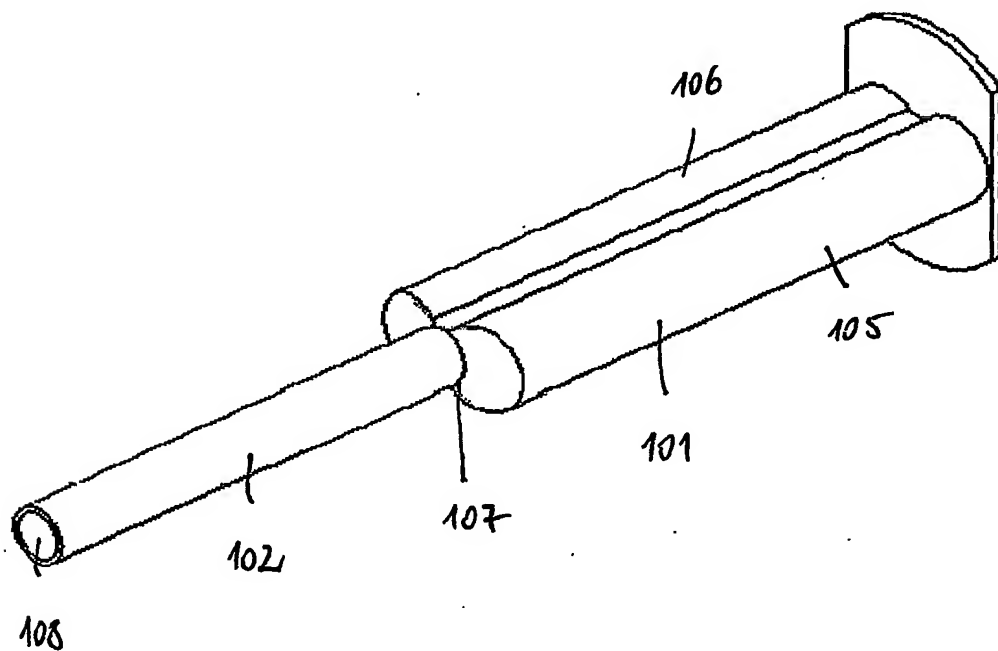


FIG. 3

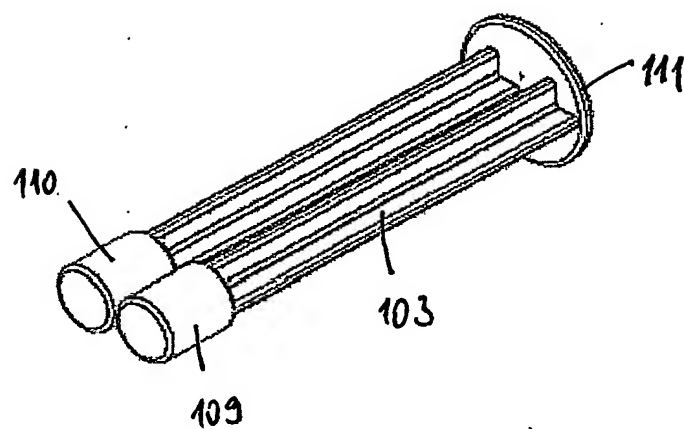


FIG. 4

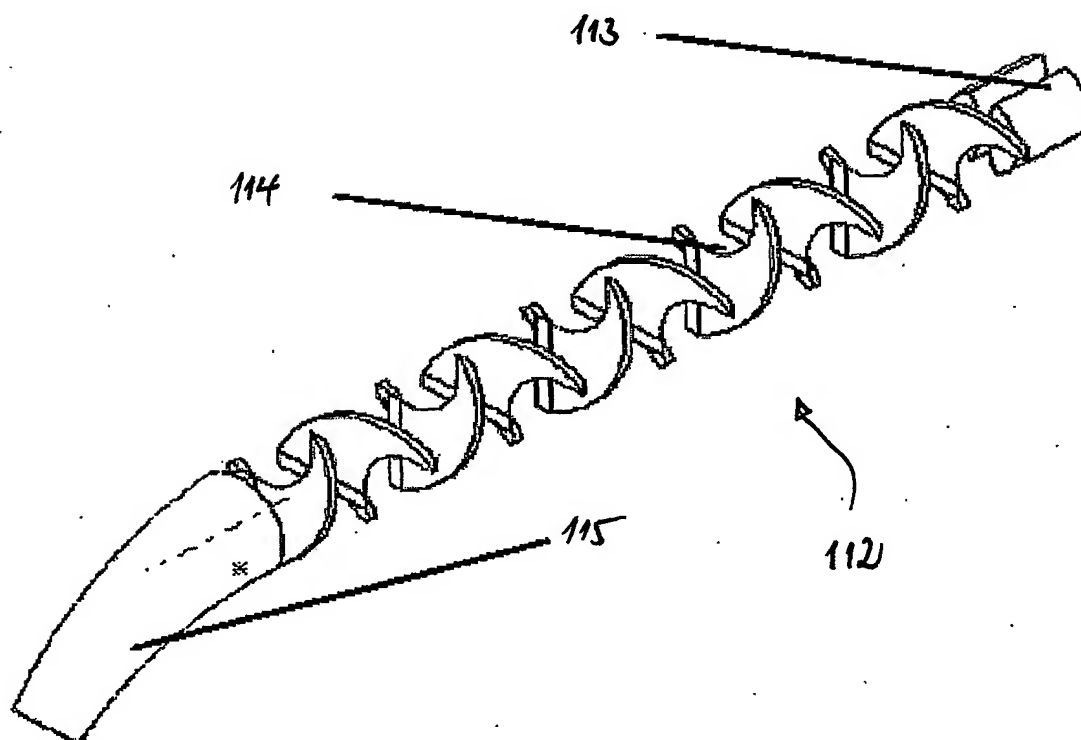


FIG. 5

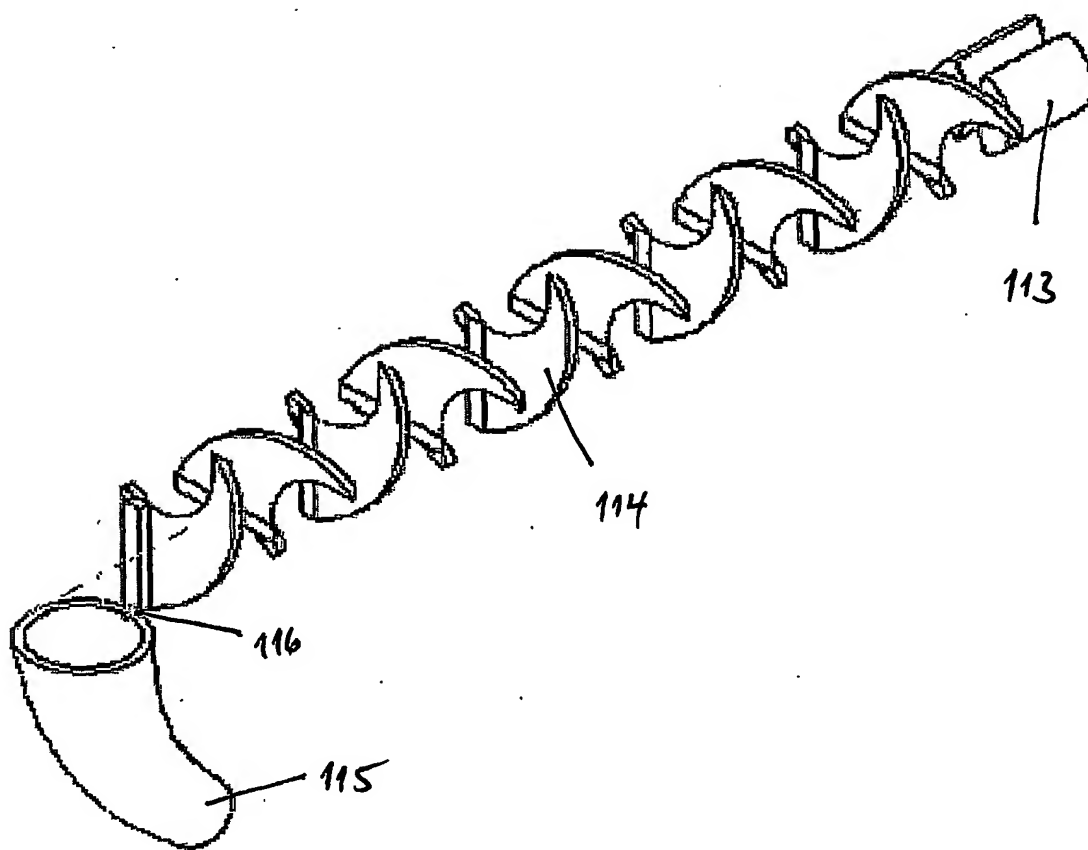


FIG. 6

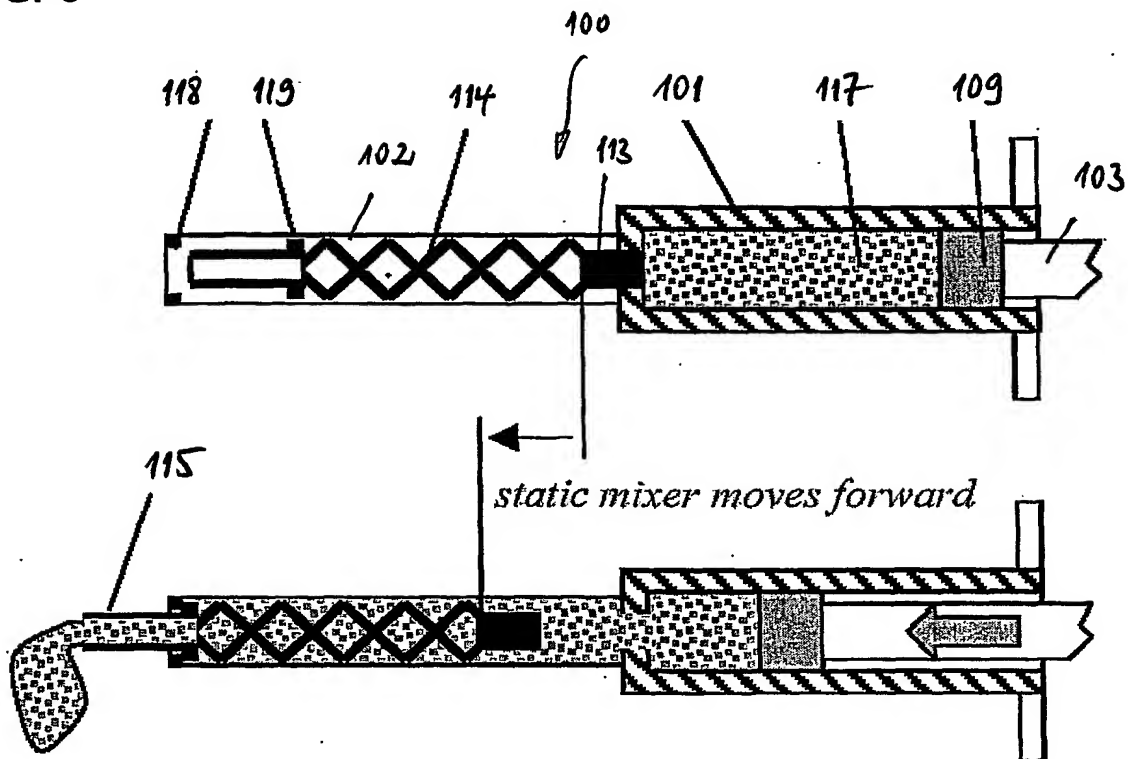


FIG. 7

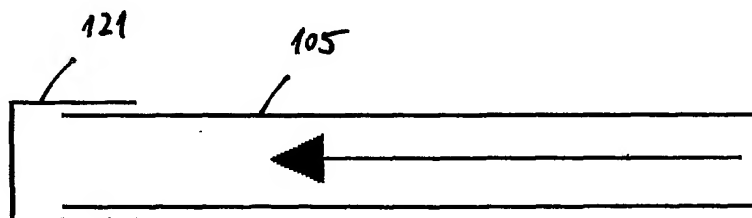


FIG. 8

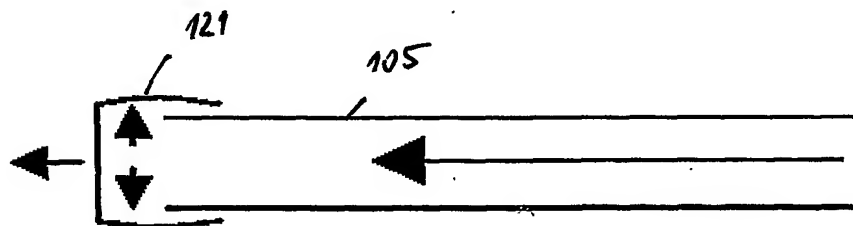


FIG. 9

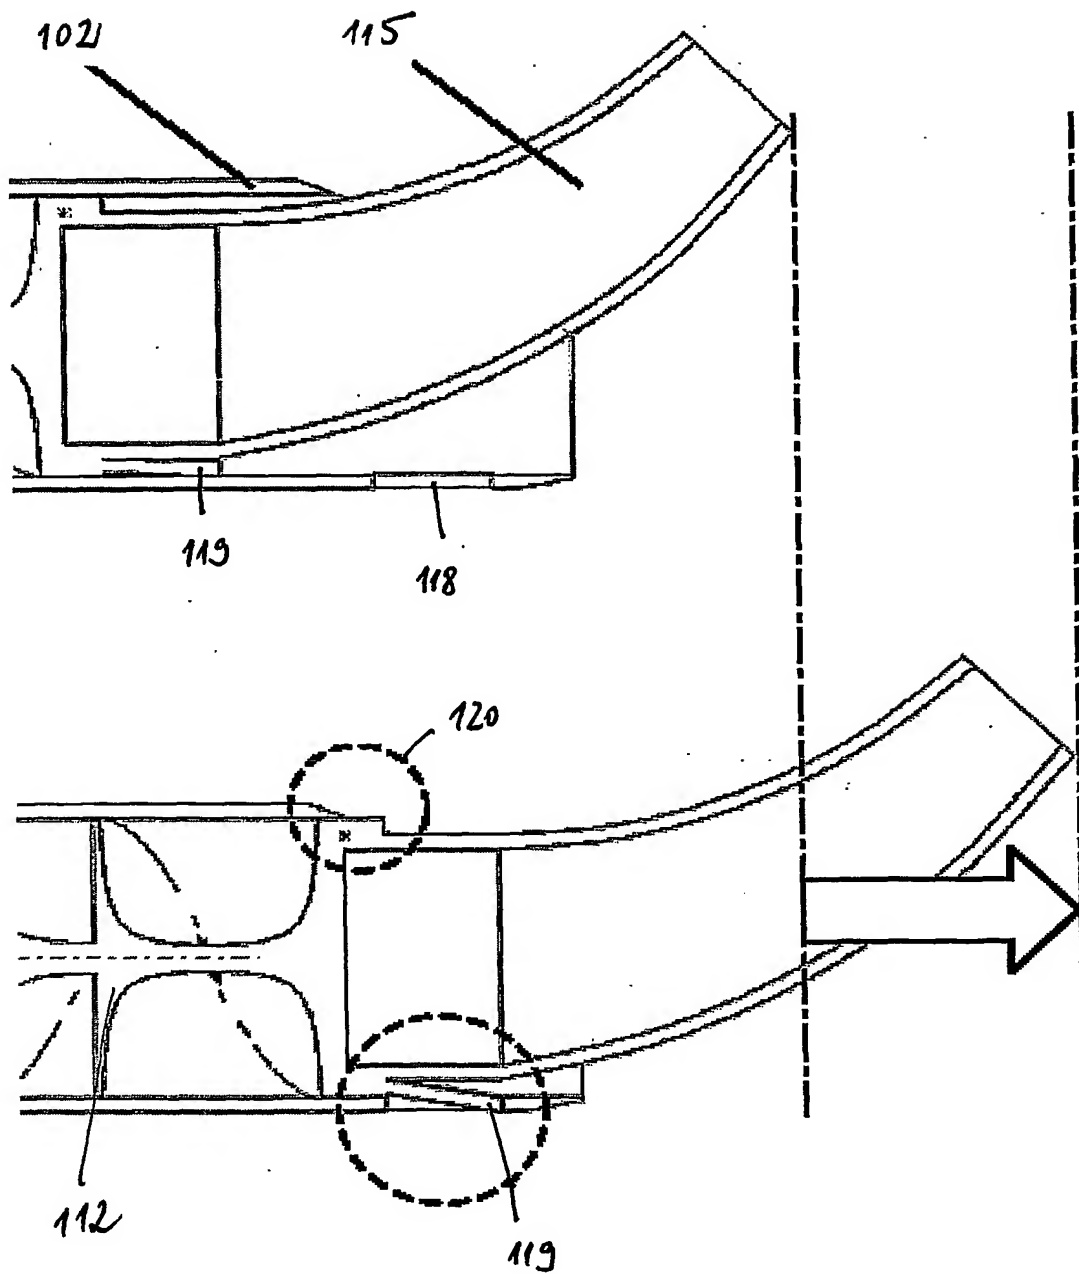


FIG. 10

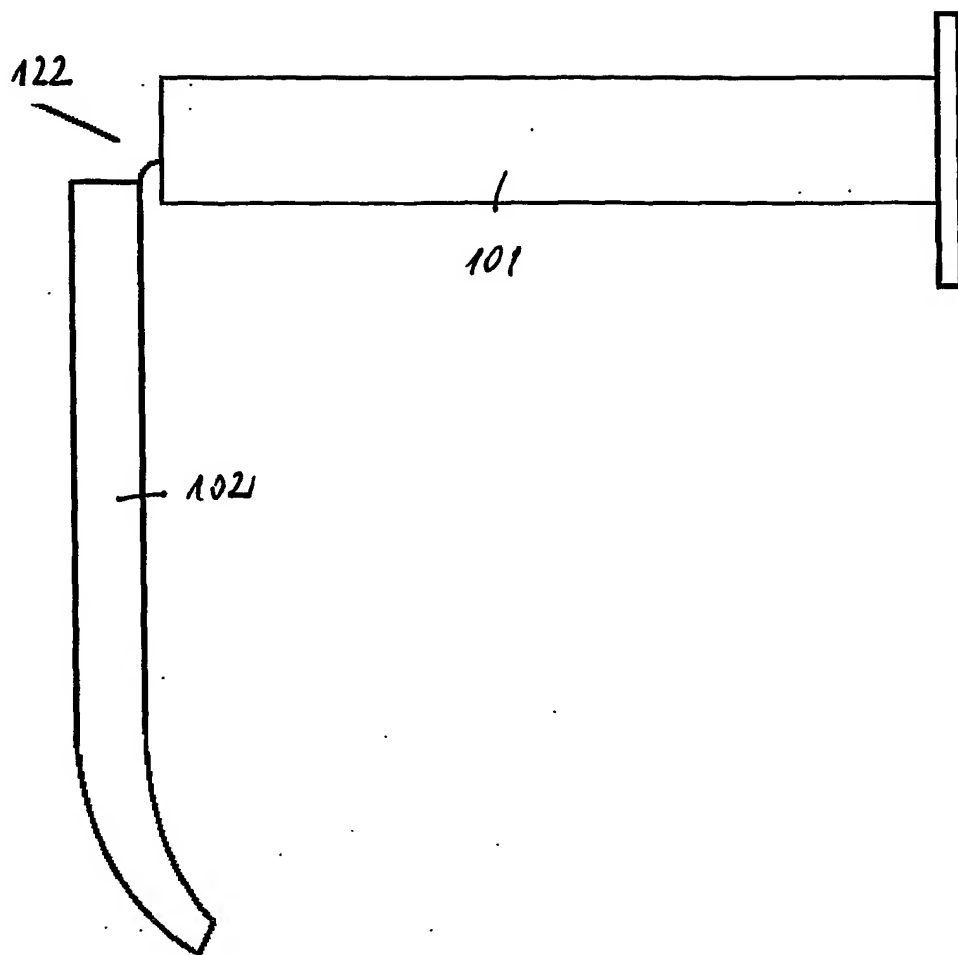


FIG. 11

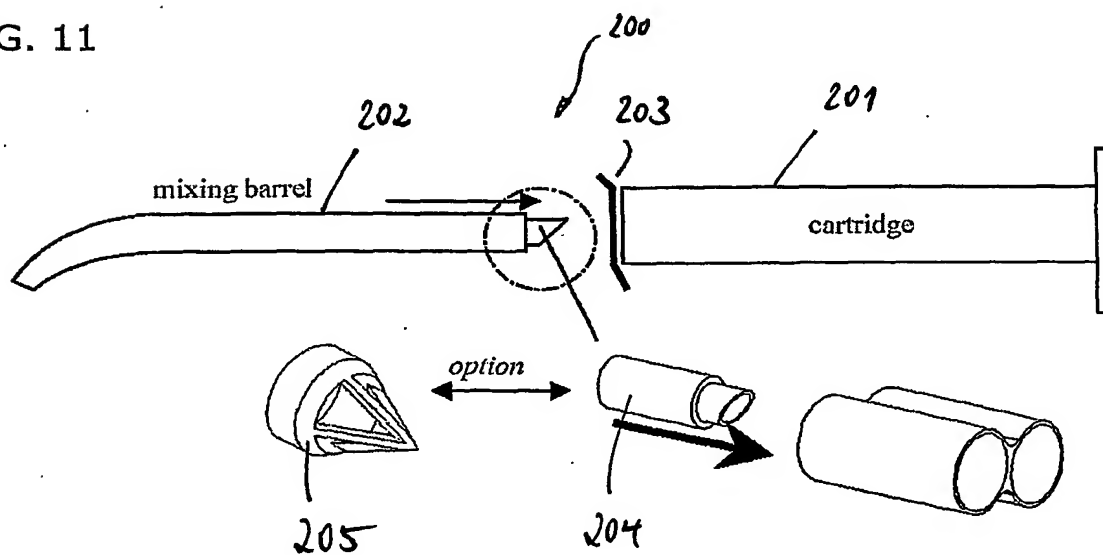


FIG. 12

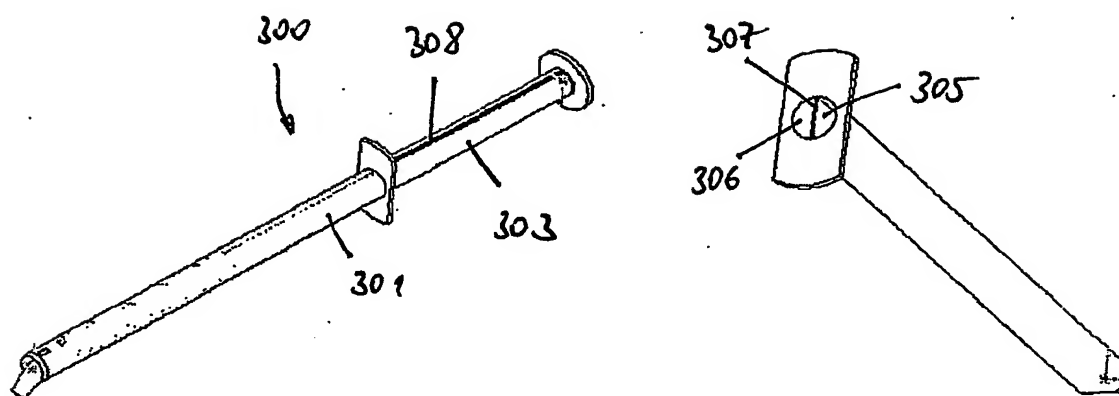


FIG. 13

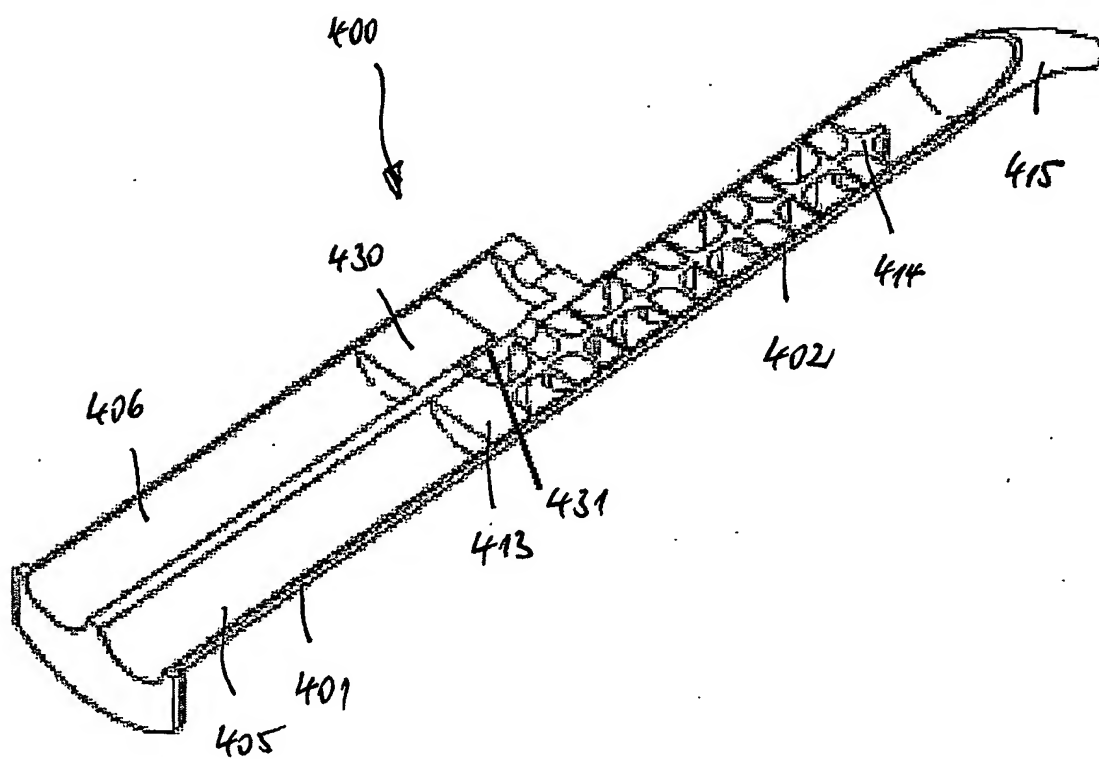


FIG. 14


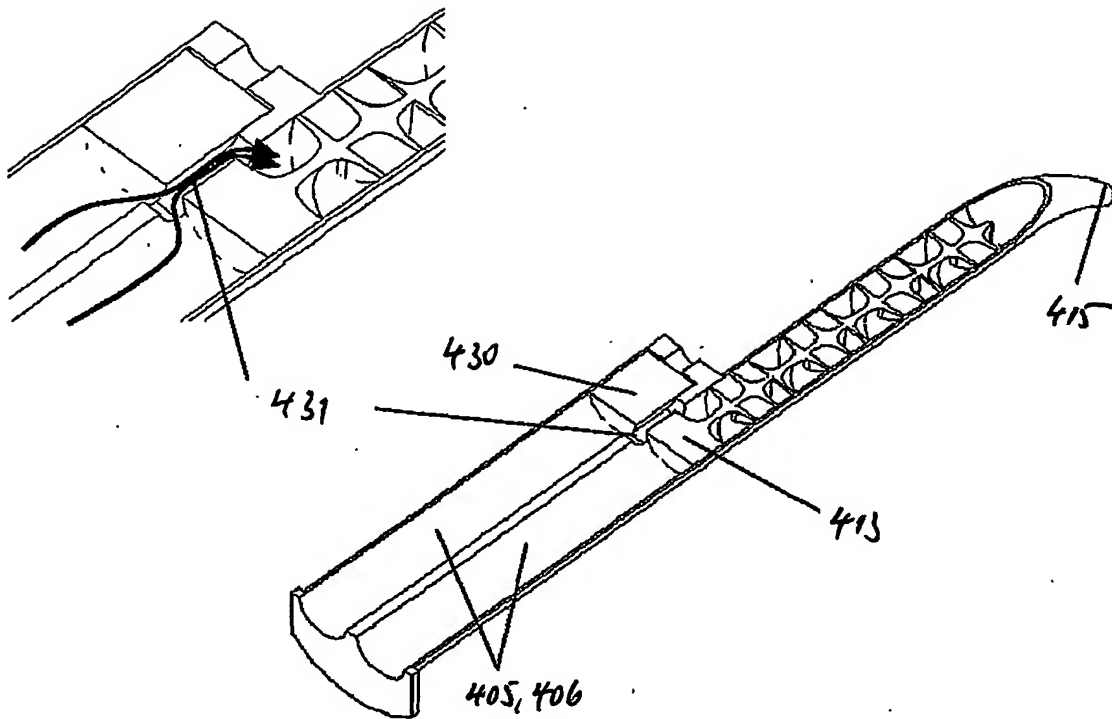


FIG. 15



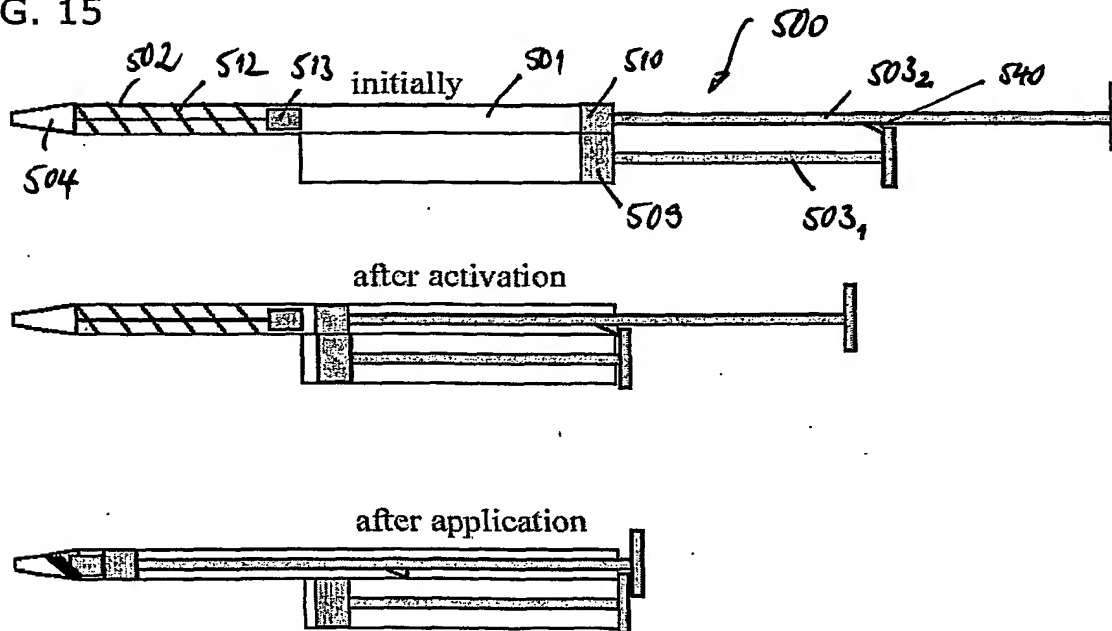

9/19

FIG. 16

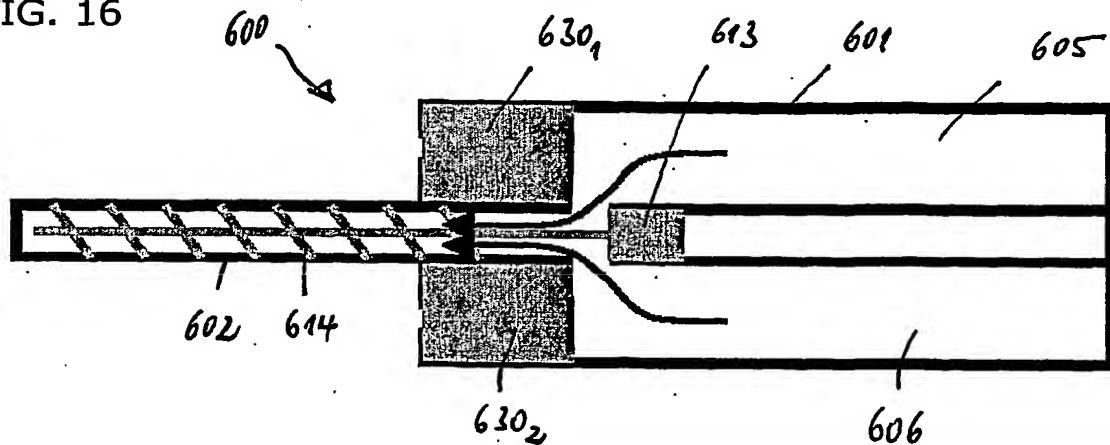


FIG. 17

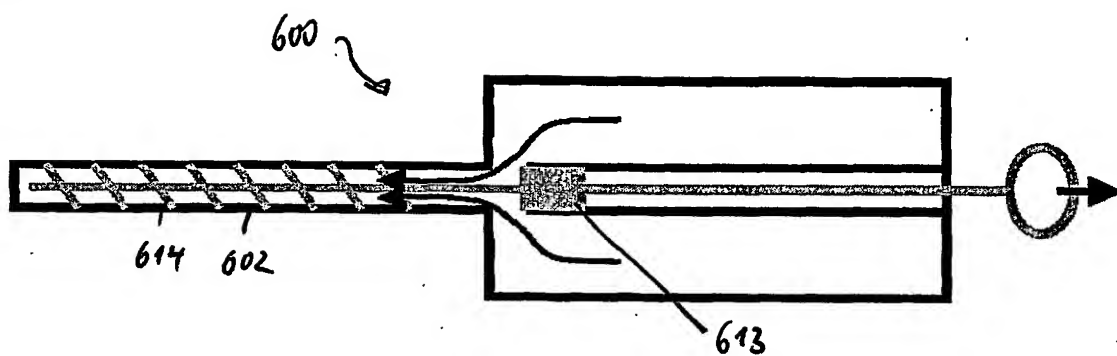


FIG. 18

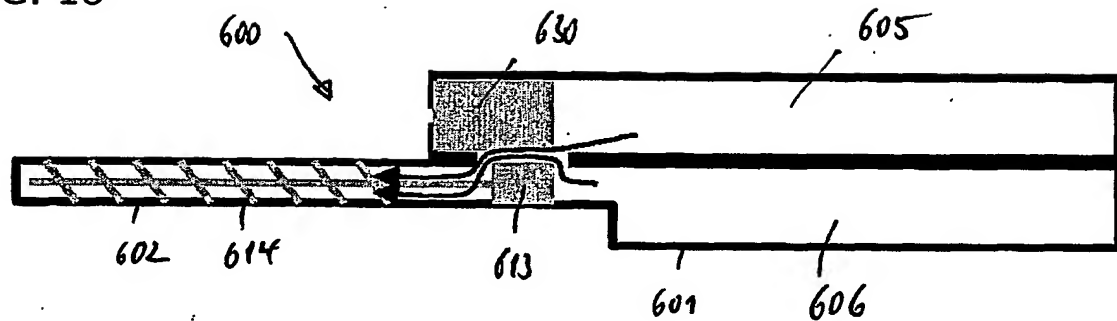


FIG. 19

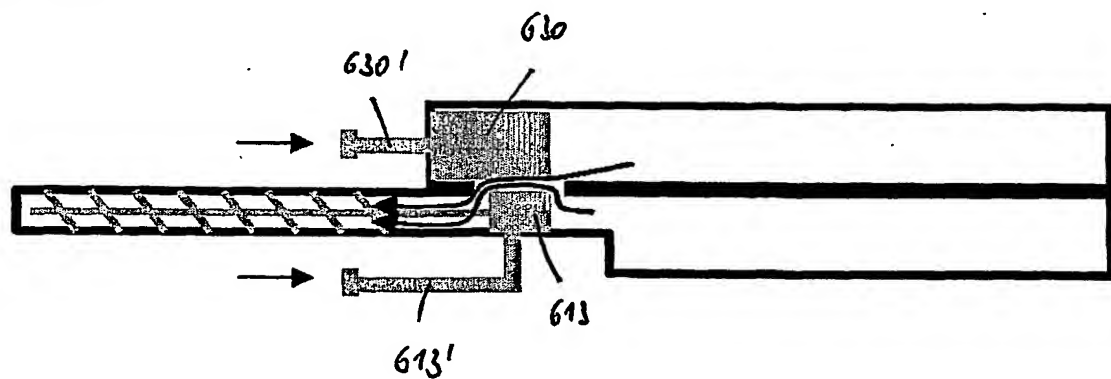


FIG. 20

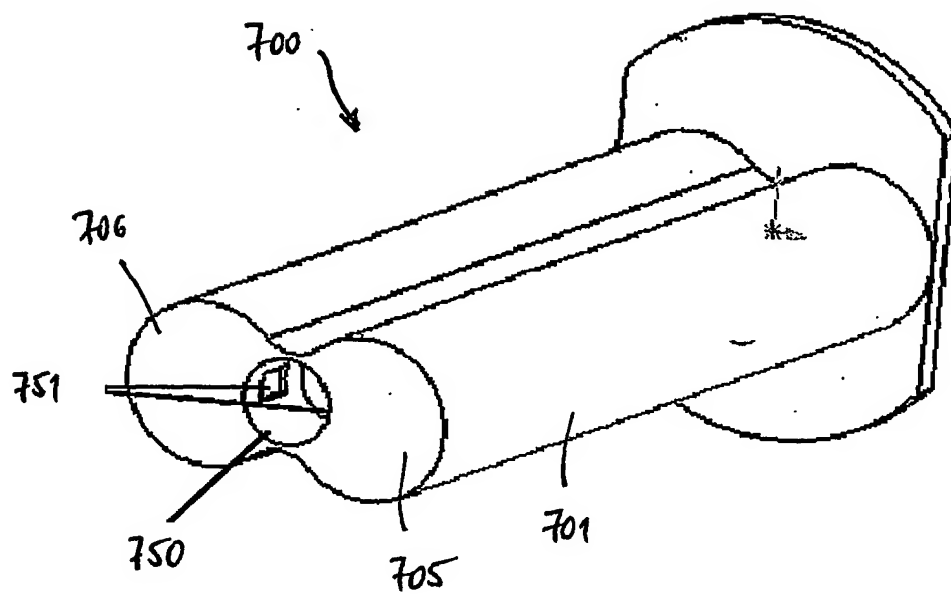


FIG. 21

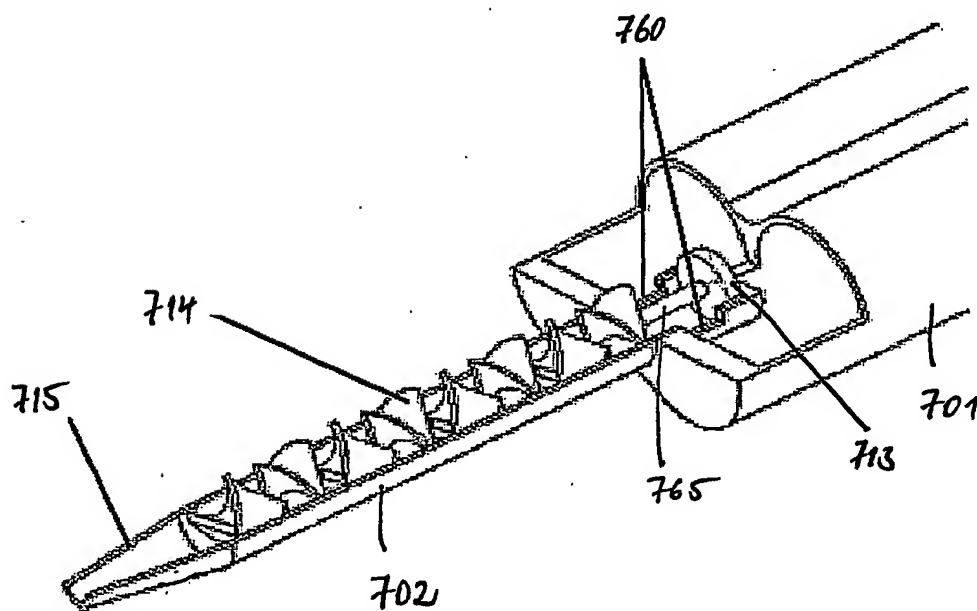


FIG. 22

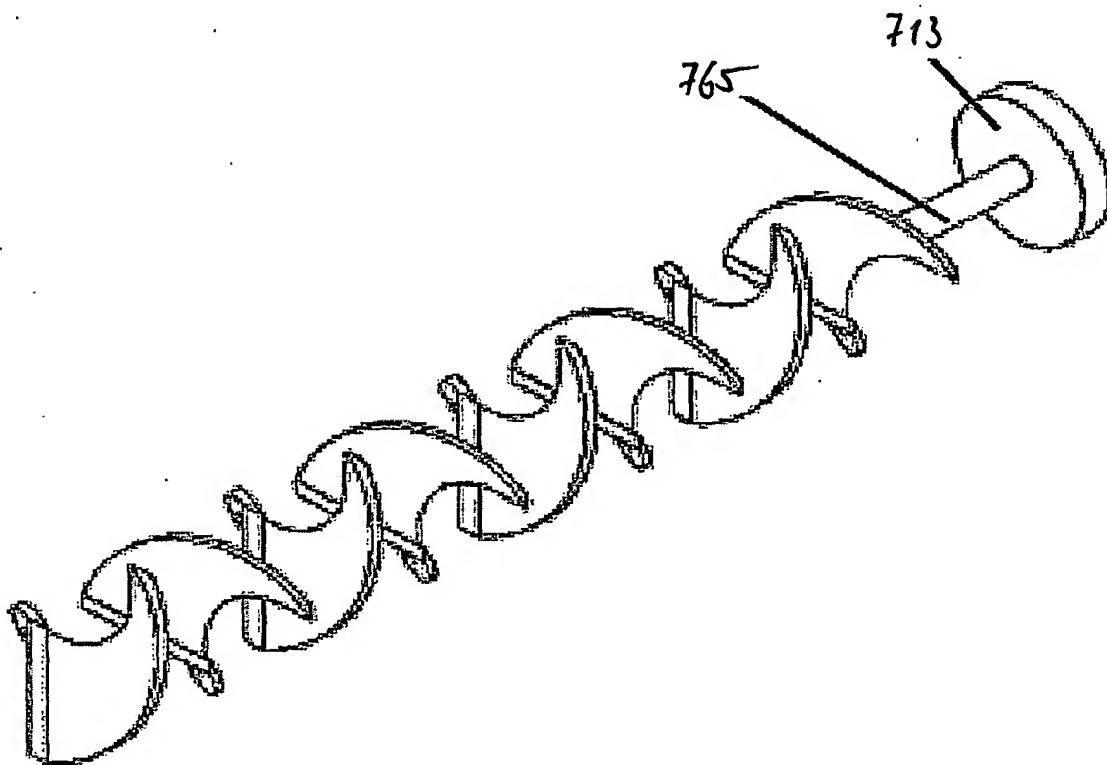


FIG. 23

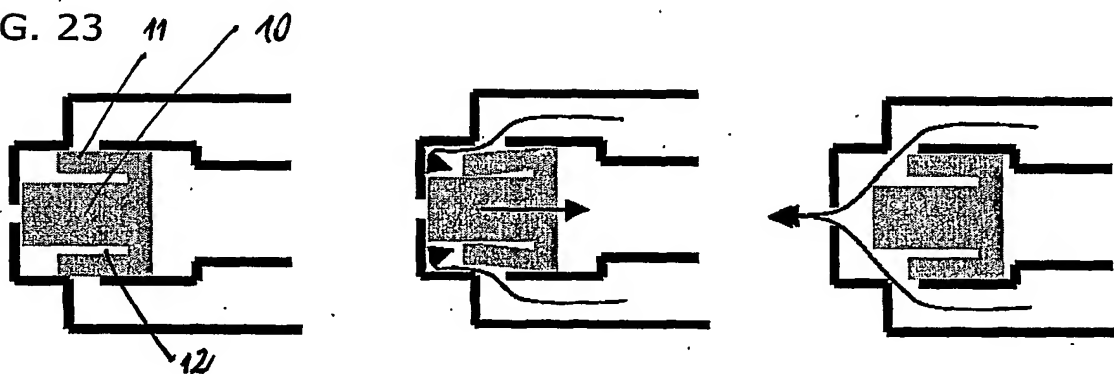


FIG. 24

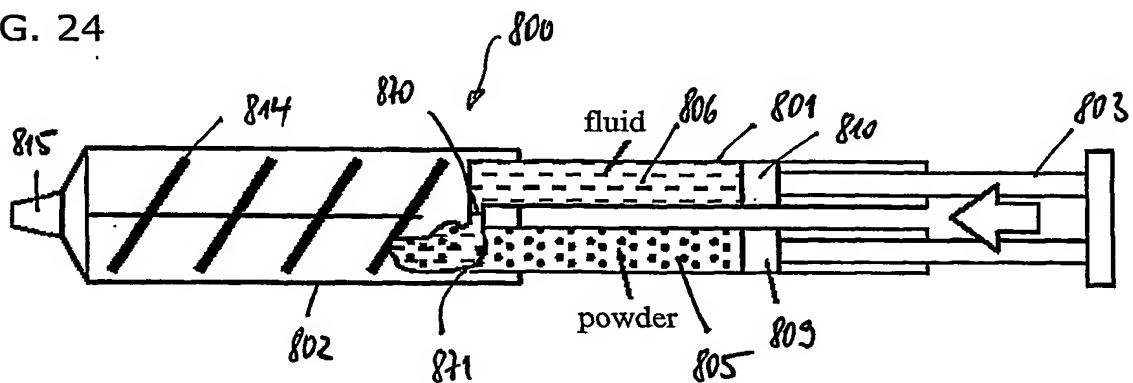


FIG. 25

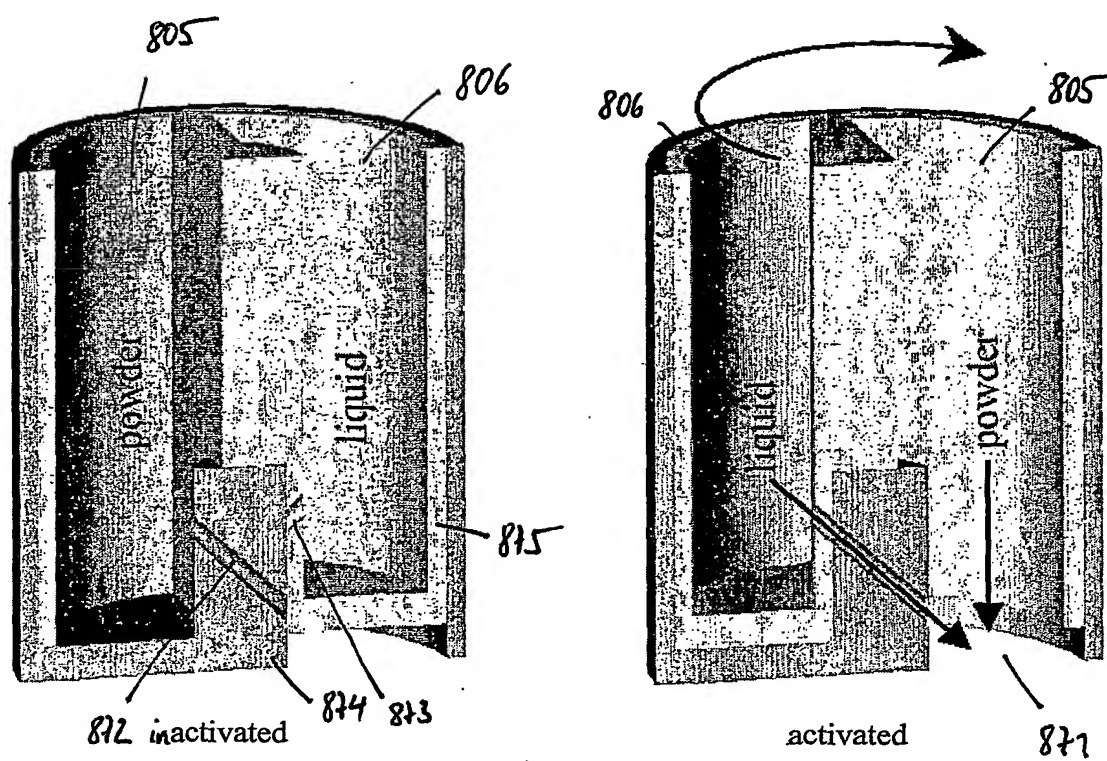


FIG. 26

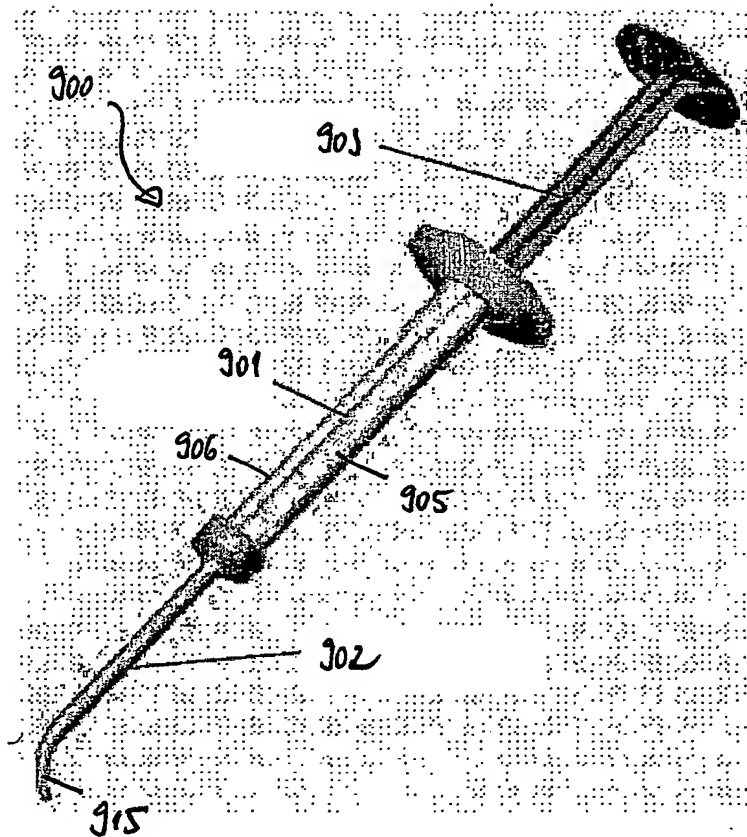


FIG. 27



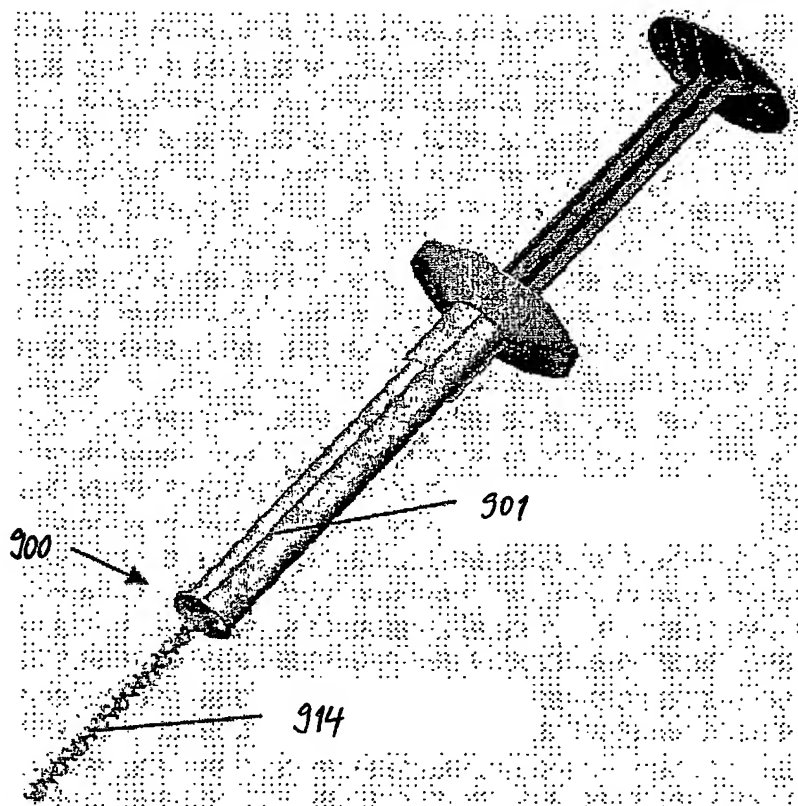


FIG. 28

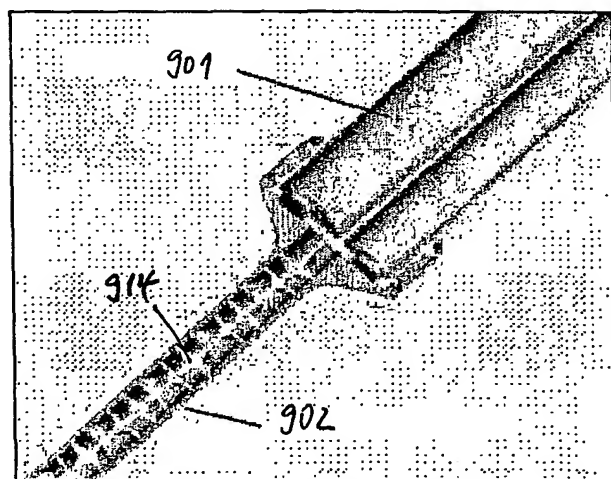

NACTIVATED  
(syringe closed, during storage)

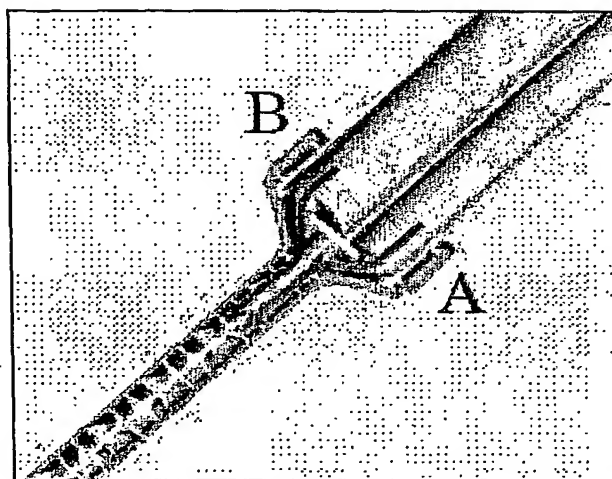

ACTIVATED  
(syringe open, for application)

FIG. 29

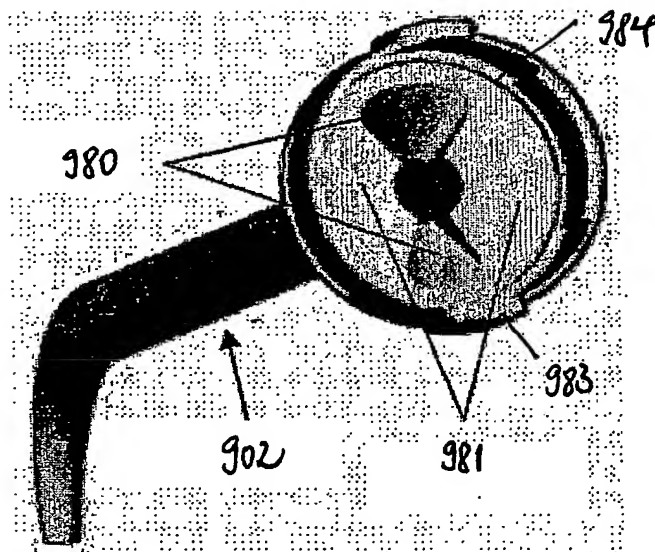


FIG. 30

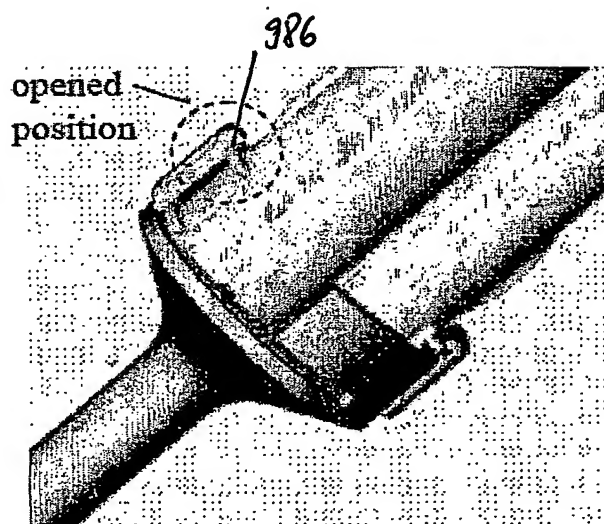
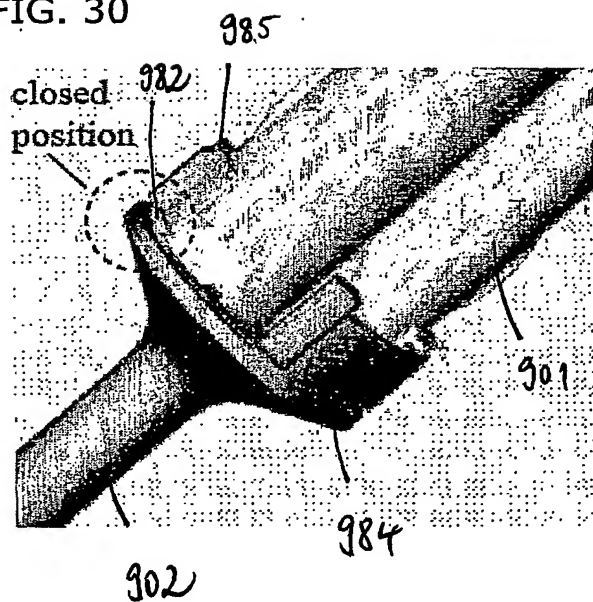


FIG. 31

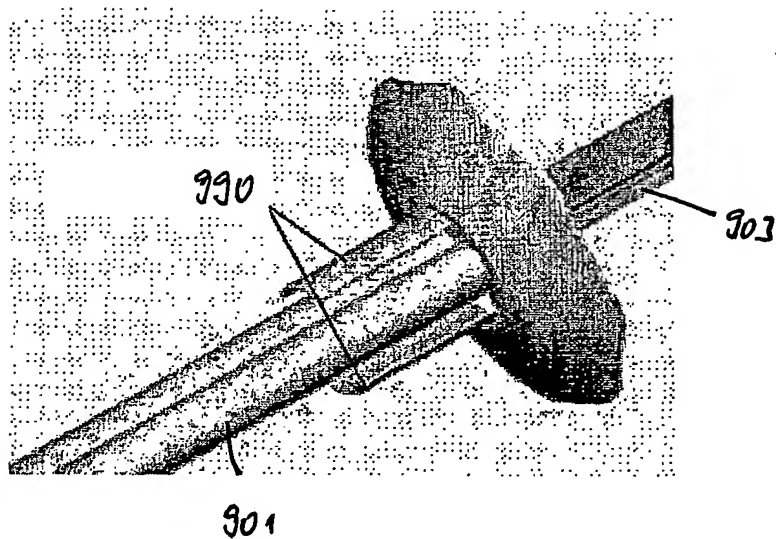


FIG. 32

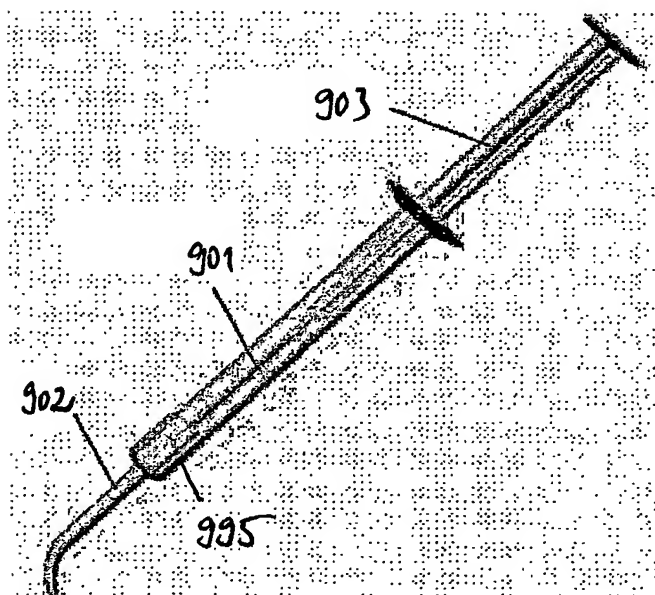




FIG. 33

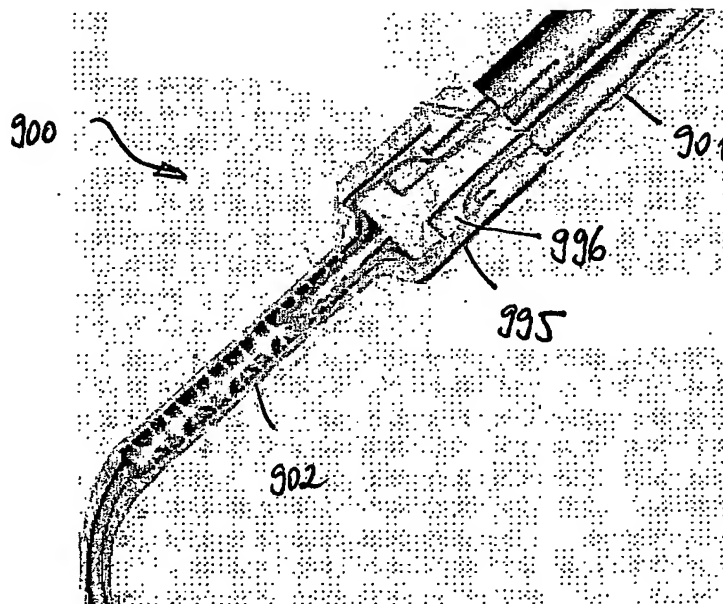


FIG. 34

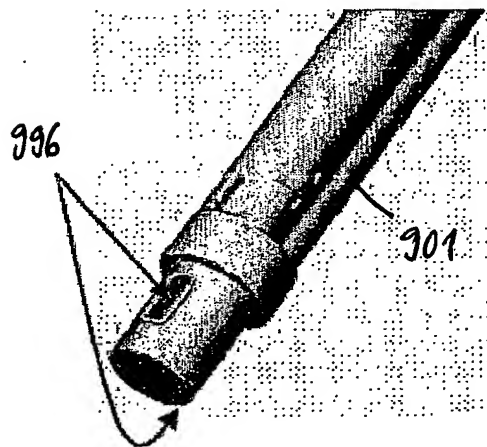


FIG. 35

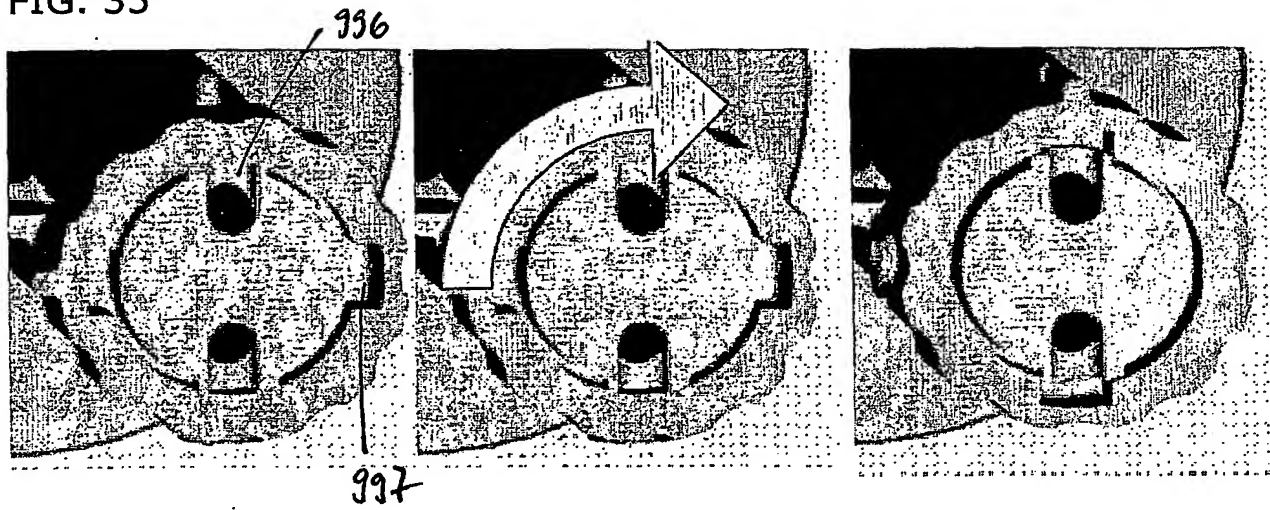


FIG. 36

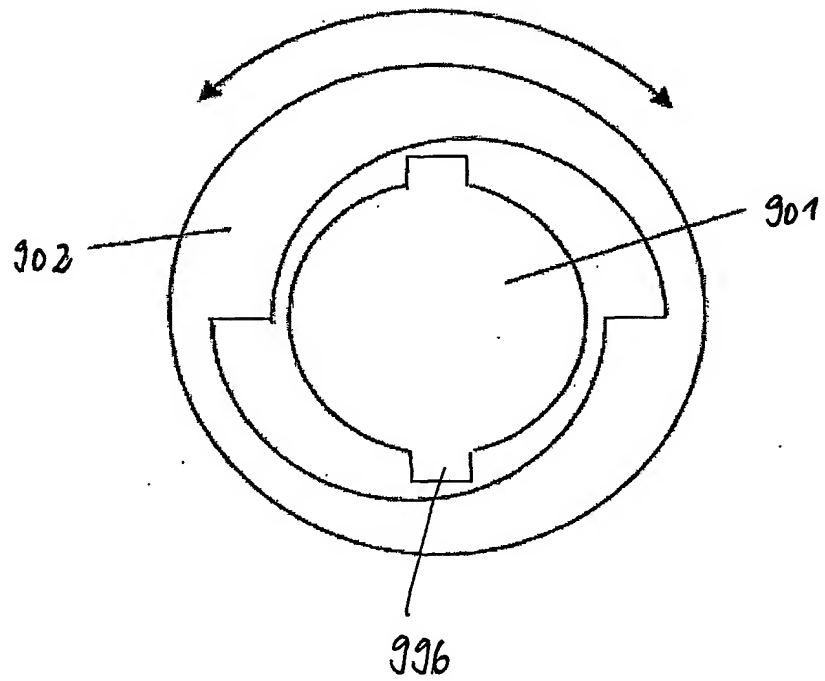


FIG. 37

